



70um 488, 561, 633, 405

| | | | |
|-------------------|------------|--------------|---------------------|
| Cytometer: | FACSriaII | User: | accDFZ |
| Cytometer Name: | FACSriaIII | Institution: | BRI COH |
| Serial Number: | P28200125 | Software: | BD FACSDiva 6.1.3 |
| Input Device: | Manual | Date: | 6/1/2015 1:09:43 PM |
| Sheath Pressure: | 70.00 | | |
| Nozzle Size: | 70 | | |
| Window Extension: | 2.00 | | |


4001111 Laser
(488nm)
ECC

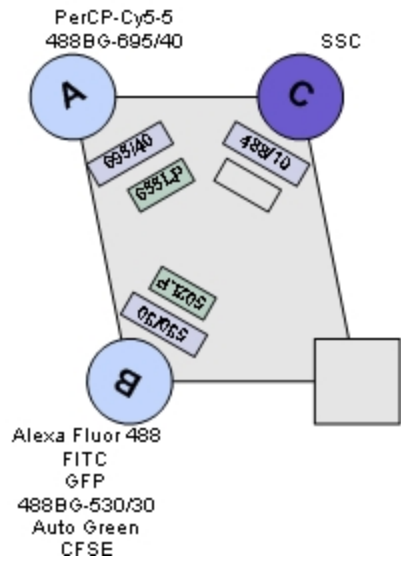


561nm Laser
(561nm)

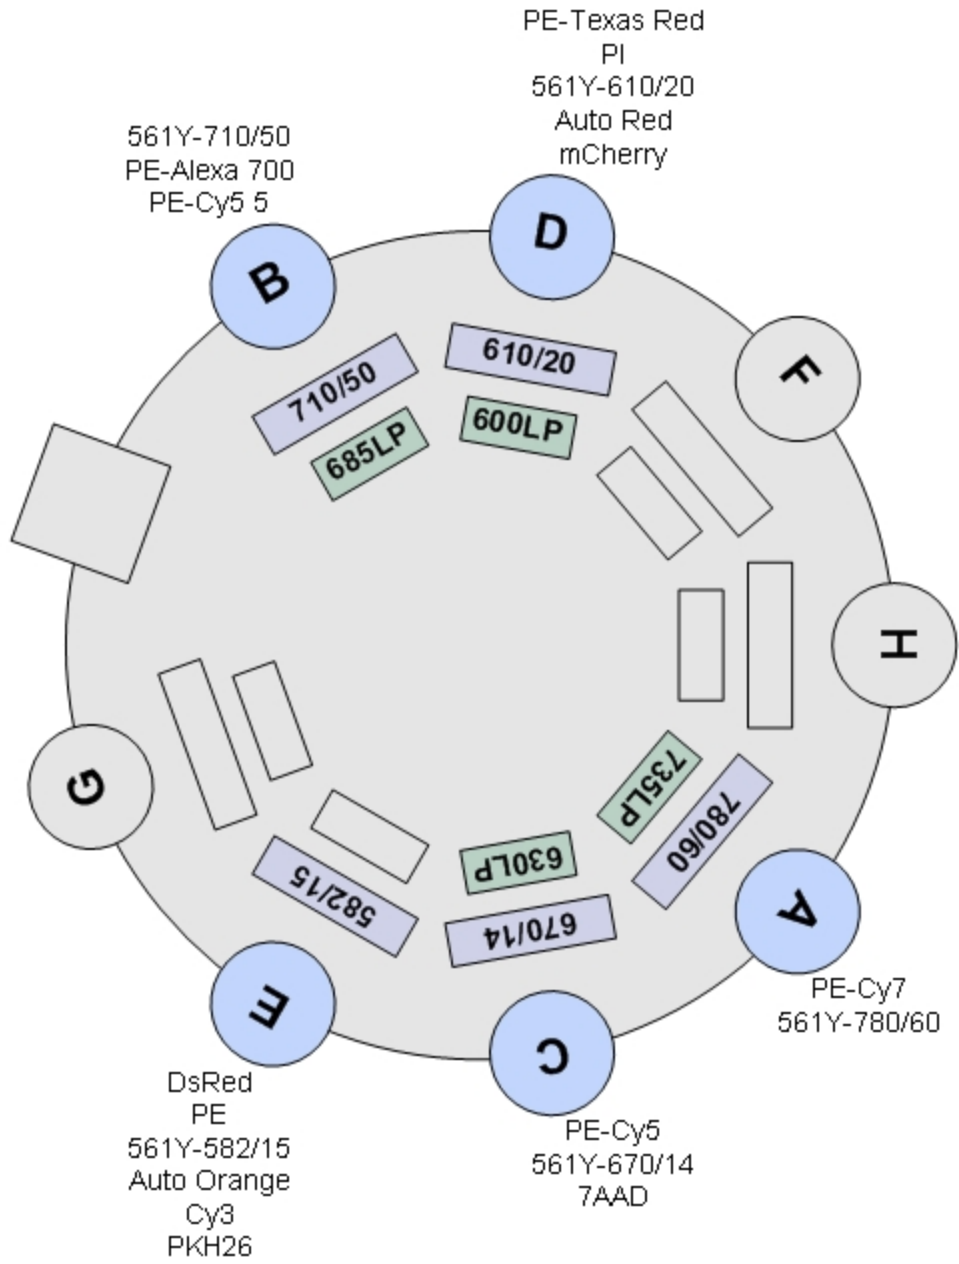

633nm Laser
(633nm)

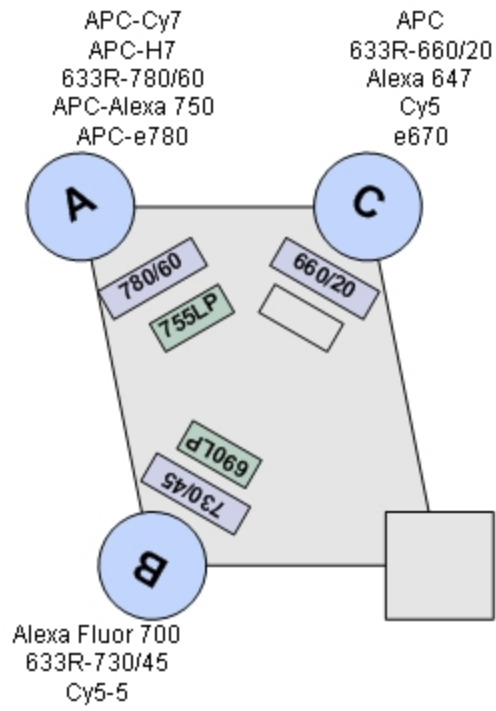

405nm Laser
(405nm)

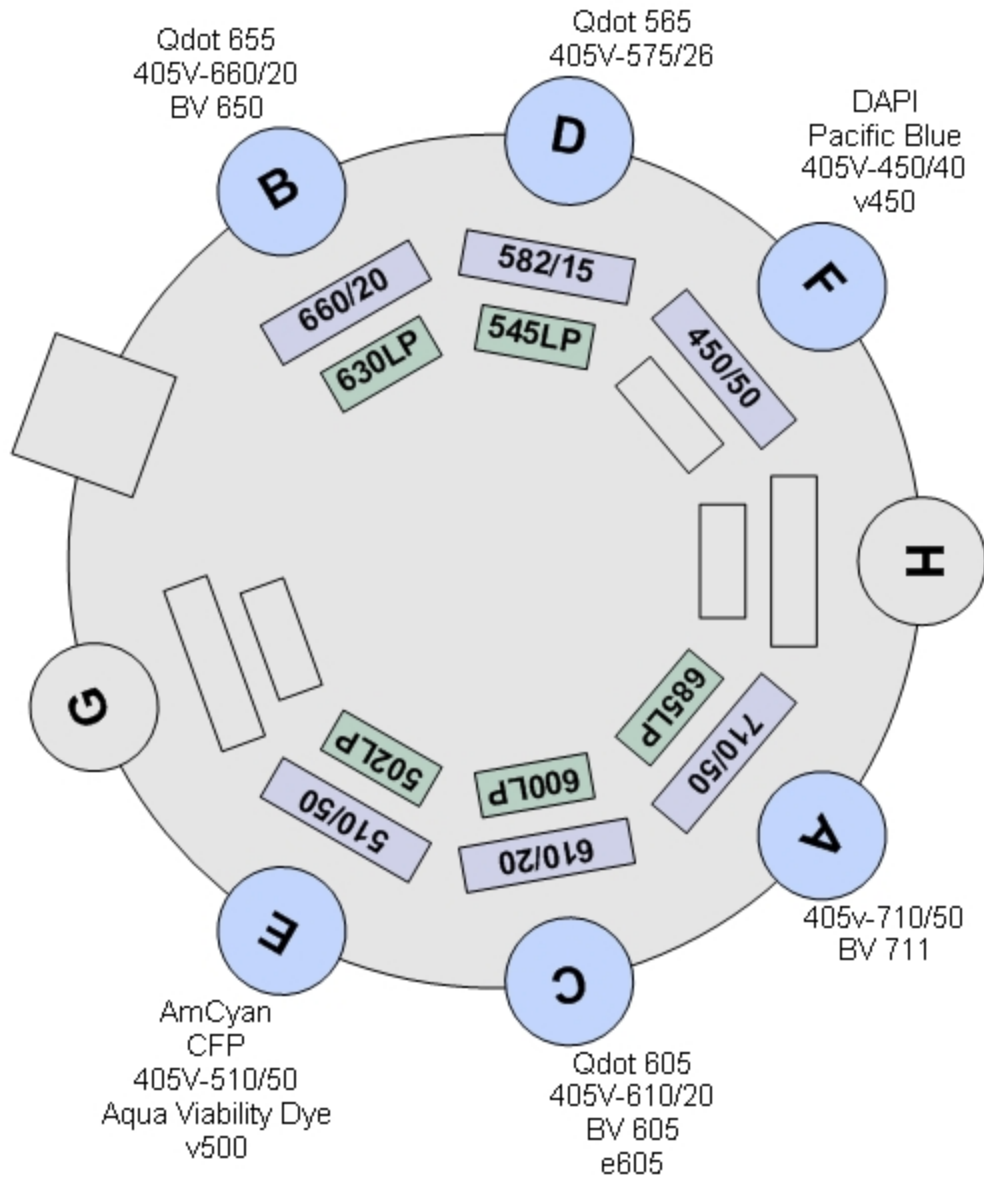

Comments: