



Jan2013 A 70psi _Standard_6 laser (1B-3R-5V-2uv-5yg-CFP)

Cytometer:	FACSAriaII	User:	Administrator
Cytometer Name:	FACSAriaII	Institution:	COH BRI
Serial Number:	P65011000025	Software:	BD FACSDiva 6.1.3
Input Device:	Manual	Date:	4/1/2013 9:55:03 AM
Sheath Pressure:	70.00		
Nozzle Size:	70		
Window Extension:	2.00		


Red Laser (640nm)

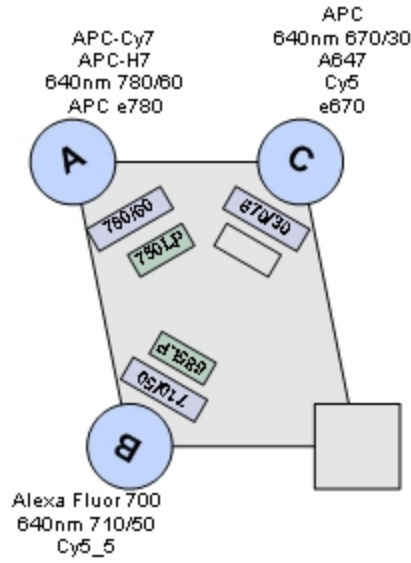

UV Laser (355nm)

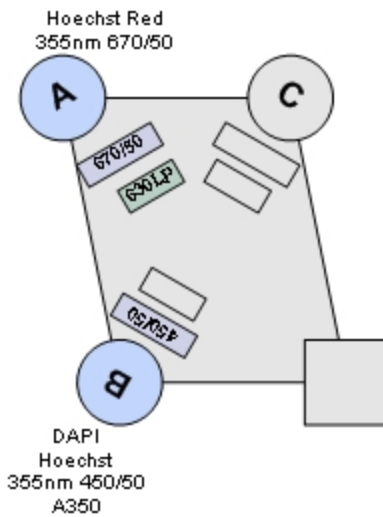


Violet Laser
(405nm)

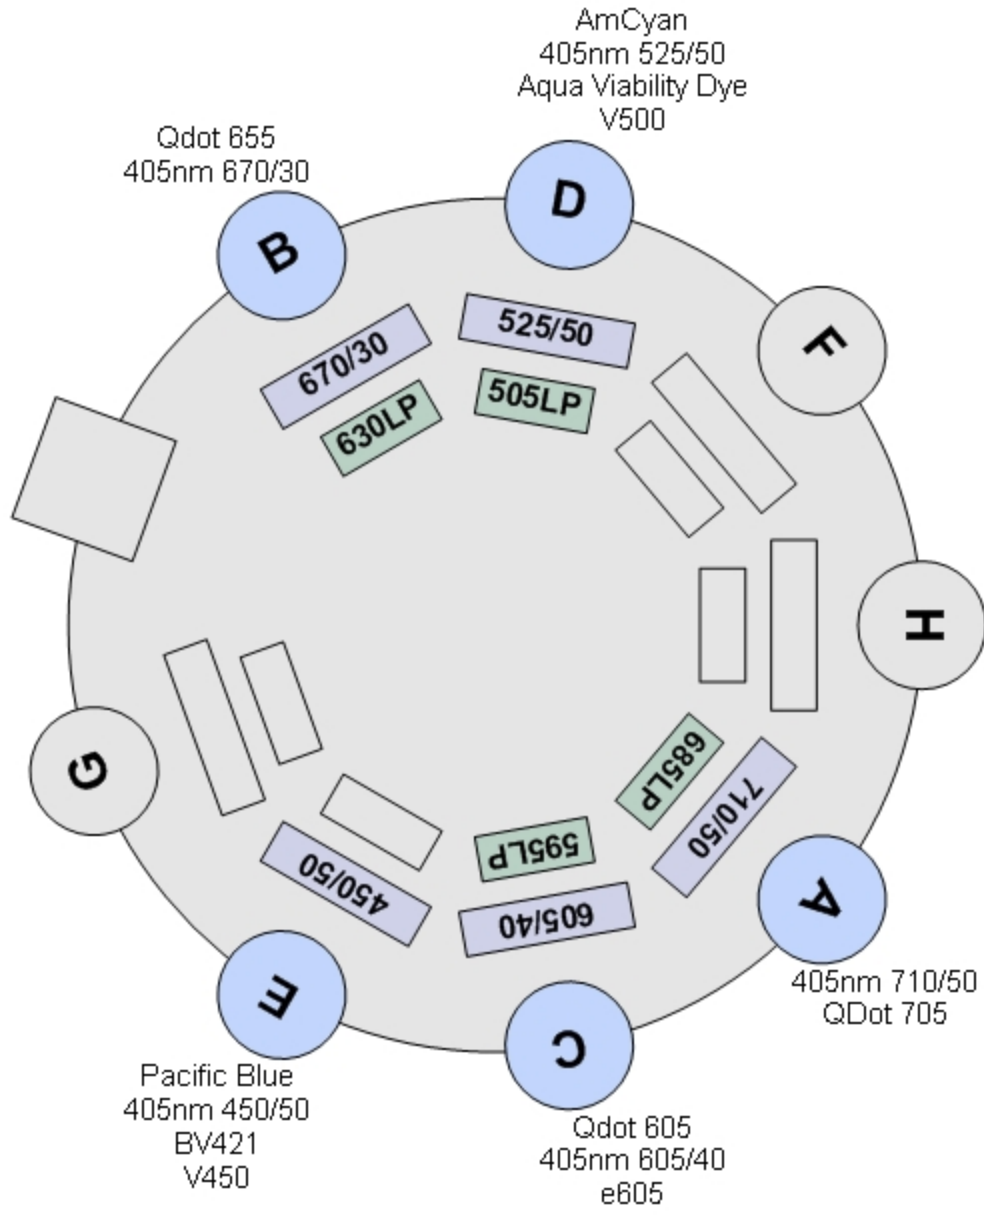


Blue Laser
(488nm)
SSC


FITC
GFP
488nm 530/30
A488
Auto Green
CFSE...

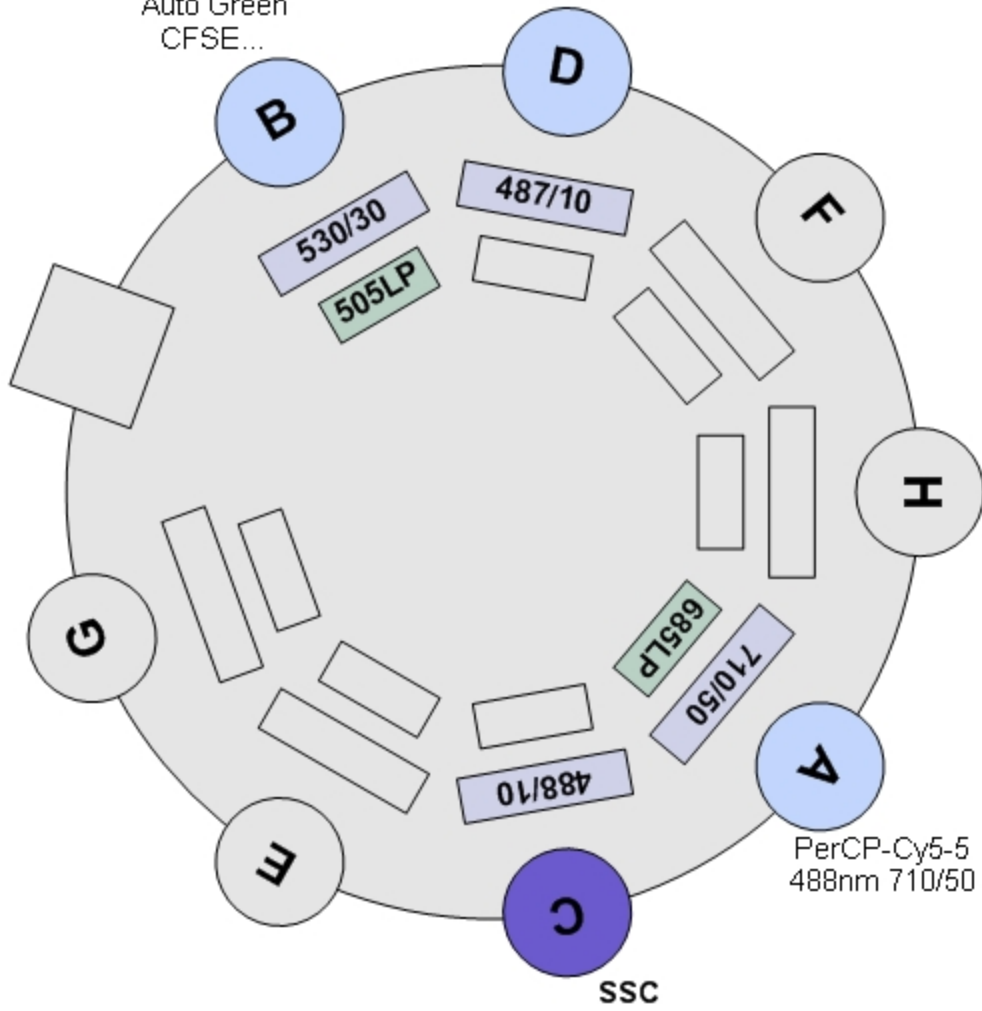

Yellow Green Laser
(561nm)

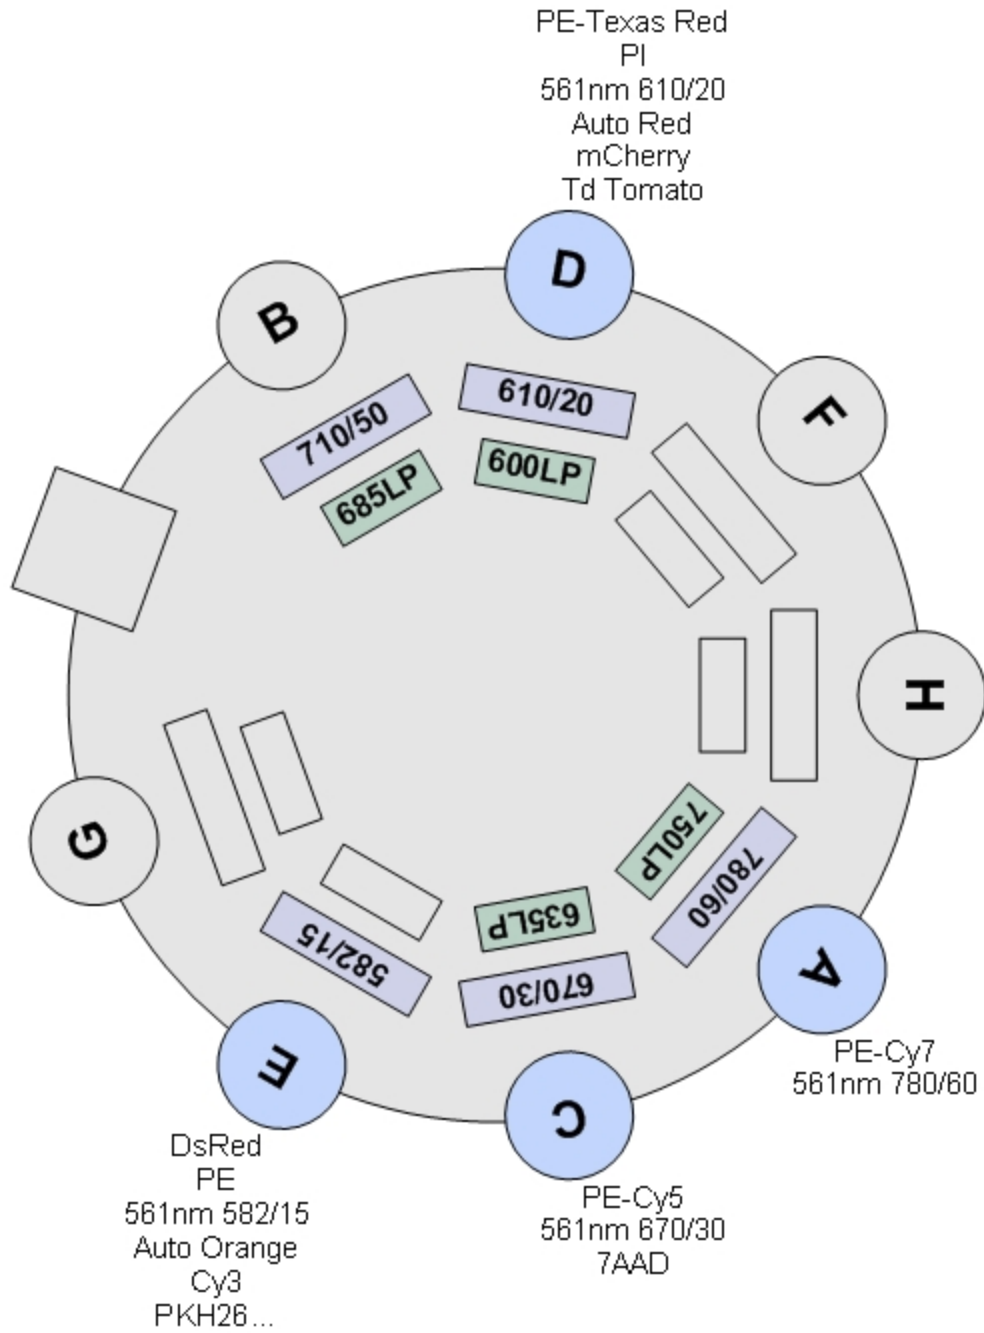

Blue Violet Laser
(445nm)

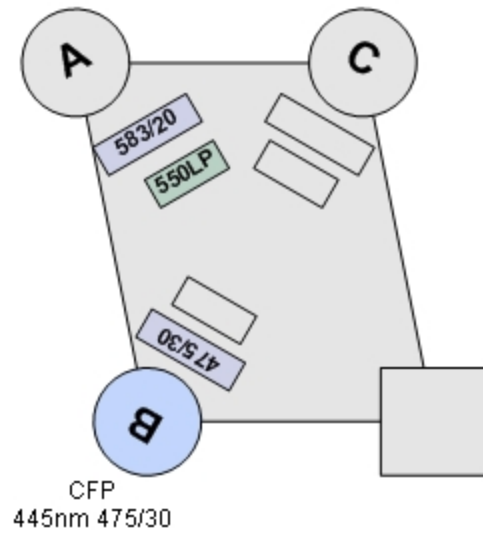

Comments:

Standard Configuration

Switch Box 3=A=PerCP-Cy5.5

Switch Box 13=A=CFP